

APPLICATION

NEXT ASS'Y

USED ON

VAR

REVISIONS

REV

DESCRIPTION

ECN

APP'D

NR

RELEASED TO DRAFTING


ECB 2907

36687


Related Drawing

No modifications permitted
without the approval of the
authorized person

PINOUT




A = POWER/INPUT
B = GROUND

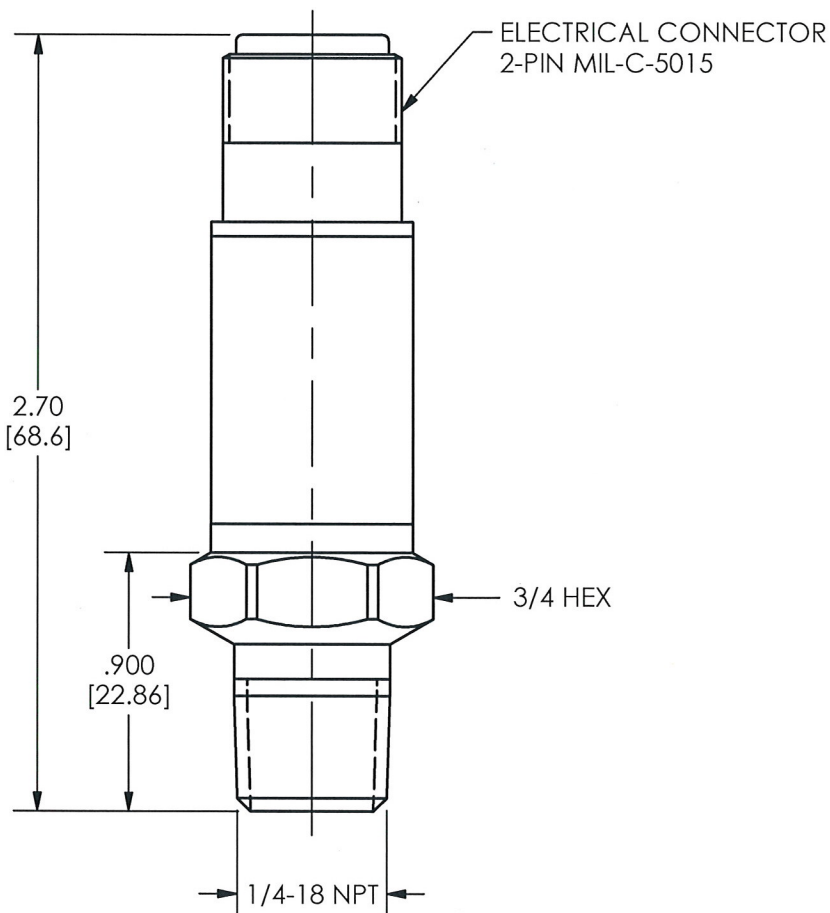

MOUNTING HOLE PREPERATION

$\varnothing .437 [\varnothing 11.10]$
X .402 [10.21] ∇ MIN
1/4-18 NPT

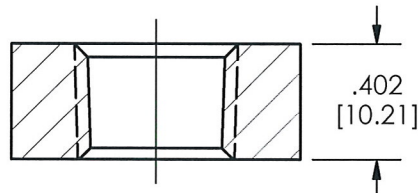

- 4.) THIS IS A SEALED ASSEMBLY AND SHOULD BE RETURNED TO THE FACTORY SHOULD SERVICE BECOME NECESSARY.
- 3.) USE PIPE JOINT COMPOUND TO ASSURE A TIGHT SEAL.
- 2.) RECOMMENDED MOUNTING TORQUE ON 3/4 HEX: 5-7 FT LBS [7-9 Nm].
- 1.) RECOMMENDED MAX INSERTION OF ADAPTOR INTO MOUNTING HOLE NOT TO EXCEED .402 [10.21].

UNLESS OTHERWISE SPECIFIED TOLERANCES ARE:

DIMENSIONS IN INCHES

DECIMALS XX $\pm .01$
XXX $\pm .005$
ANGLES ± 2 DEGREES

DIMENSIONS IN MILLIMETERS
[IN BRACKETS]

DECIMALS X ± 0.3
XX ± 0.13
ANGLES ± 2 DEGREES

FILLETS AND RADII
.003 - .005

FILLETS AND RADII
[0.07 - 0.13]

DRAWN

ECB

2907

MFG

PRR

2-9-07

CHK'D

ECB

2907

ENGR

JF

2-9-07

APP'D

NJL

2/9/07

SALES

DPC

2/9/07

TITLE

INSTALLATION DRAWING
MODEL 121A41,A44,A45
PRESSURE SENSOR



PCB PIEZOTRONICS INC.

3425 WALDEN AVE. DEPEW, NY 14043
(716) 684-0001 E-MAIL: sales@pcb.com

CODE
IDENT. NO.
52681

DWG. NO.

36687

SCALE: 1.5X

SHEET 1 OF 1